



Software for the Molecular Imaging Community.

ec2software.com

400 Apgar Drive, Suite I, Somerset, NJ 08873
P: 800 851 0025 F: 732 356 8746
info@ec2software.com



Nuclear Medicine Software

Version 22 Installation Guide

Current & New Network User

This installation guide is intended for customers who are upgrading from a previous version of software and for new customers.

Included are the recommended hardware specifications a summary of the new features and sample screens to guide you through the installation.

Introduction

Welcome

Thank you for being a loyal user of ec² Software Solutions. The following pages will guide you through the installation process. If you need help at any time during the installation, please contact our [technical support](#) team. We appreciate your business and look forward to serving you.

Table of Contents

- Guide to New NMIS/RMIS Features.....3
- Guide to New BioDose Features.....5
- Hardware Requirements.....6
- Proxy Server Requirements.....7
- Pre-Installation Checklist.....8
- Server Installation.....9
- Workstation Installation.....16
- Software Registration.....19
- Old to New BioDose Conversion.....22
- Pre-Installation Checklist.....23
- Conversion Instructions.....24
- Contact Information.....25

Guide to New NMIS/RMIS Features

What's New in NMIS Version 22

1. Vendor Orders Enhancement (NMIS)

We improved our Orders module by allowing the entering, displaying and submitting the **Referring Physician** when placing Vendor Orders.

2. Kit QC Report Enhancement (NMIS)

We improved our Hot Lab Reports module by adding an export functionality to the Hot Lab QC Chromatography report.

3. Instrument QC Report Enhancement (NMIS)

We improved our Health Physics Reports module by adding a **% Deviation** column which is displayed when a deviation is out of range of validation.

4. Audit Trail Report Enhancement (NMIS)

We improved our Reports module by adding an audit trail entry for failed user login attempts.

5. Hot Lab Inventory Preferences Enhancements (NMIS)

- **Change Unit to Bulk Dose:** Users or administrators only can change inventory from unit to bulk dose in the scheduler.
- **Product Approval/Release - Hospital:** Kits can now be approved in-house by a supervisor prior to being used to dose a patient.

6. Patient Reporting Program Improvement (NMIS)

We replaced Microsoft Word DSO framer, which was no longer supported, with DevExpress controls ensuring no change in functionality.

7. Only Allow Rx #s to Show for Draw Dose Preference (Combo NMIS/RMIS)

We added a **Show only inventory processed with Rx #s** option which can be set to only show unit doses processed with Rxs in the scheduler.

8. Ga68 Generator Elution (RMIS)

We improved our Elute module functionality of the Ga68 Generator and added four new cold kits.

- Illucix
- PSMA
- PSMA-11
- Locametz

9. **MAA Reduced Particle from MAA Cold Kit (RMIS)**

We improved our Kit Prep module and added the ability to make MAA Reduced Part from MAA - Cold Kit.

10. **Invoice Detail Report Enhancement (RMIS)**

We enhanced our Pharmacy Reports module and now include an **NDC Code** and **NDC Manufacturer** optional fields.

11. **Inventory Screen Labels (RMIS)**

We enhanced our Hot Lab module and added the option to print labels directly from the inventory screen.

12. **Product Approval/Release - Pharmacy (RMIS)**

We improved our Hot Lab Inventory Preferences where kits can now be approved in-house by a supervisor prior to a dose being dispensed to the patient.

Guide to New BioDose Features

What's New in BioDose Version 22

1. Vendor Orders Enhancement

We improved our Orders module by allowing the entering, displaying and submitting the **Referring Physician** when placing Vendor Orders.

2. Kit QC Report Enhancement

We improved our Hot Lab Reports module by adding an export functionality to the Hot Lab QC Chromatography report.

3. Instrument QC Report Enhancement

We improved our Health Physics Reports module by adding a **% Deviation** column which is displayed when a deviation is out of range of validation.

4. Audit Trail Report Enhancement

We improved our Reports module by adding an audit trail entry for failed user login attempts.

5. Hot Lab Inventory Preferences Enhancements

- **Change Unit to Bulk Dose:** Users or admins only can change inventory from unit to bulk dose in the scheduler.
- **Product Approval/Release - Hospital:** Kits can now be approved in-house by a supervisor prior to being used to dose a patient.

6. Patient Reporting Program Improvement

We replaced Microsoft Word DSO framer, which was no longer supported, with DevExpress controls ensuring no change in functionality.

Hardware Requirements

Below are the requirements to run this software for a network user license. Please check to ensure that your hardware meets these requirements. If you have any questions or concerns about the requirements, contact our [technical support](#) team and we'll be happy to review your hardware with you.

Server Hardware

Processor	Intel Core i5
Memory	8GB RAM
Screen Resolution	1280 x 1024 (required minimum)
Hard Drive	1 TB
Optical Drive	DVD for software installation
Backups	External hard drive, USB flash drive or shared network folder

Workstation Hardware

Processor	Intel Core i5 or better
Memory	8GB RAM
Screen Resolution	1280 x 1024 (required minimum)
Hard Drive	500 GB

Operating System

Windows 10 TH1 1507 or greater
Windows Server 2016 or greater

Internet Access

Recommended for:

- Downloading periodic program updates
- Accessing ec² software remote support portal
- Online ordering where available

Proxy Server Requirements

The services that allow you to send orders online, download software service packs and access our remote support service depend on the software being allowed to make outbound calls to the Internet. If your facility uses a proxy server to access the Internet, several functions of the Nuclear Medicine Information System (NMIS), Radiopharmacy Management Information System (RMIS) or BioDose software could be blocked. Our software is not proxy aware, so the following exceptions will be needed.

The calls from the software are outbound only. We would prefer the exception to be added using the URL rather than the IP address wherever possible. Outbound calls are made from the application itself and therefore the end user will not be able to authenticate for the proxy server. Please add an exception to bypass authentication.

Ports

80 and 443

URLs

1. For Online Ordering (OLO) the following will be used:

199.233.63.164 **www.ec2softwareservices.com**

2. For Remote Support the following will be used:

199.233.63.142 **support.ec2software.com**

3. Service Pack and software downloads will use:

199.233.63.135 **ec2software.com**
<https://www.dropbox.com>

4. Online ordering with some pharmacies can also require the following:

Independents nuclear-pharmacy.com
Jubilant Radiopharma onlineorder.triadisotopes.com

Pre-Installation Checklist

Before you Begin

Making sure that your hardware is adequate to run our software is extremely important. For [hardware requirements](#) information please refer to that section in this guide.

You should have received the NMIS version 22.x DVD along with this installation guide. Please check that the facility name on the disk is correct. If it is not, please contact our [technical support](#) team before continuing.


Important Points: Current User


1. Shut down any programs that are running. Antivirus software can slow down the installation or prevent it from finishing. Disable any screen savers that could disrupt the installation.
2. The software installation could take up to 60 minutes. Please give yourself plenty of time to complete the process.
3. You may be asked to restart your computer several times during the installation. Please restart whenever requested to do so.
4. You must be logged in as an administrator to install NMIS. It is important that you use the same administrator login after each restart until the program tells you the installation was successful.

Important Points: New Install


1. Please perform a backup of your data before you begin the upgrade process.
2. Shut down any programs that are running. Antivirus software can slow down the installation process or prevent it from finishing. Disable any screen savers that may disrupt the process.
3. The upgrade will take about the same amount of time if you are coming from version 14 or an earlier version. You should be able to complete the upgrade in under 1 hour in most cases.
4. If you are on version 14.x or older please note that the folder name will change. You will not be able to install to the existing NMISSQL folder. Because we are upgrading so many of the core components with this version, we want to leave the old folder untouched in case we need to go back to it for any reason.

Server Installation

1. **Insert the disk** labeled with your facility name and “Software Version 22.x” into the disk drive.
2. Double click on **Computer** on the desktop and locate the disk drive. Look for the label **ec2_22.xx_Cust#xxxxxx** and double click on it.
3. Double-click on the  **setup.exe** file.
4. The **Welcome** screen will be displayed. Click **Next**.

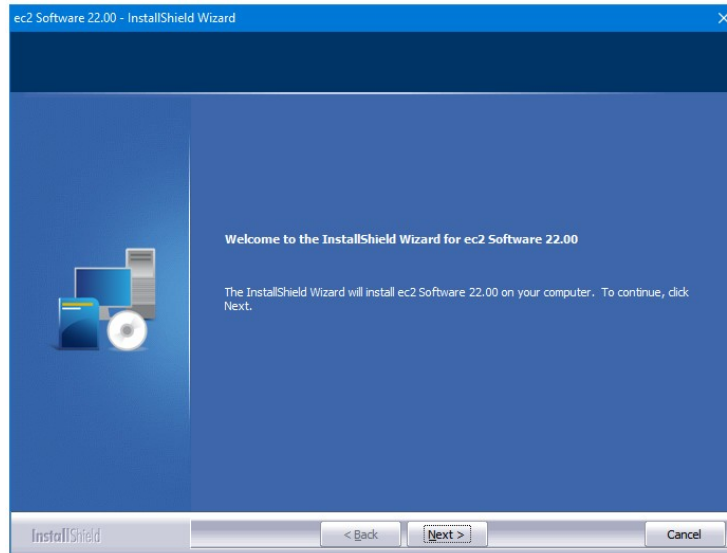


5. The installation program will examine your computer for all required components. If all required components are installed, you will move to step 8. If there are missing components, the below screen will be displayed listing them.

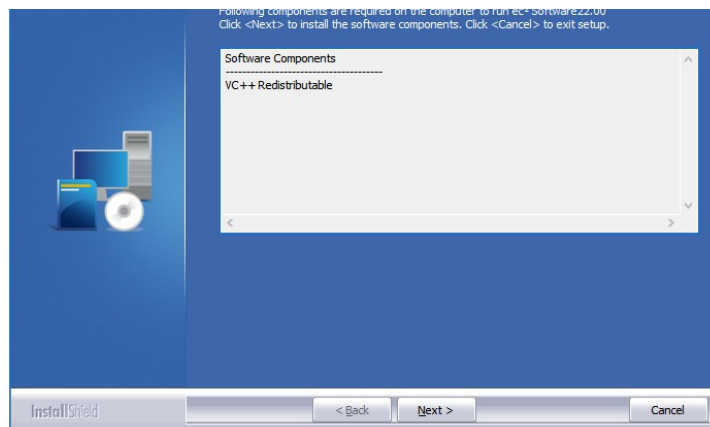


Server Installation (continued)

- The installation program will install any missing components. Click **Next** to continue. Follow the screen prompts and restart when necessary. Click **Yes** on the below message to continue.

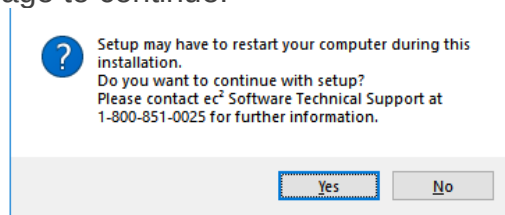


- Once all components have been installed, the **Welcome** screen will be displayed. Click **Next** to continue.
- On the **License Agreement** screen select the **I accept the terms of the license agreement** radio button then click **Next** to continue.

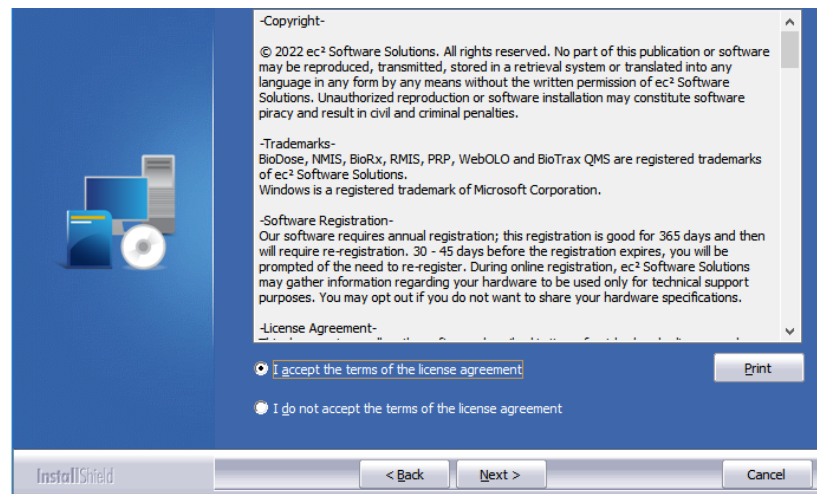


Server Installation (continued)

9. On the **Choose Installation Type** screen select **Express Server** to install on the **C:** drive and **Custom** to install on a different drive.

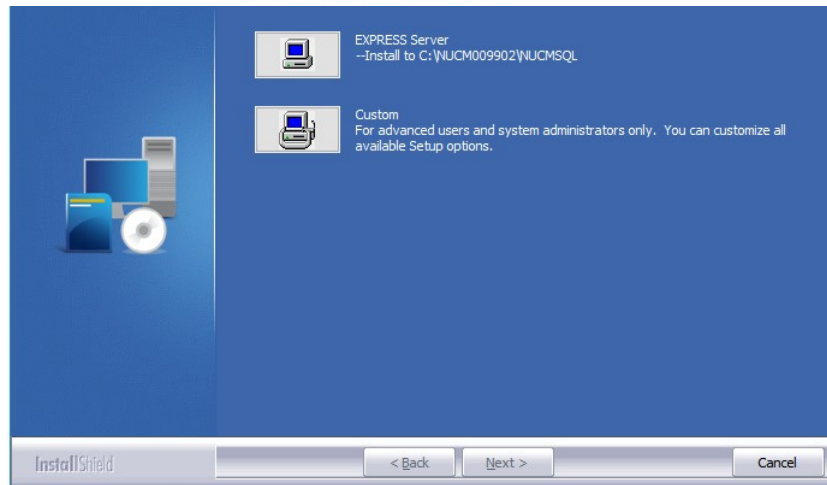


10. Click **Yes** on the below message to continue.


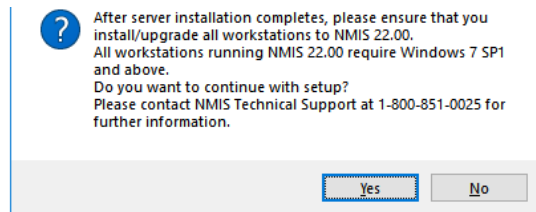


Server Installation (continued)


11. The program will copy the installation files while the below screen is displayed.

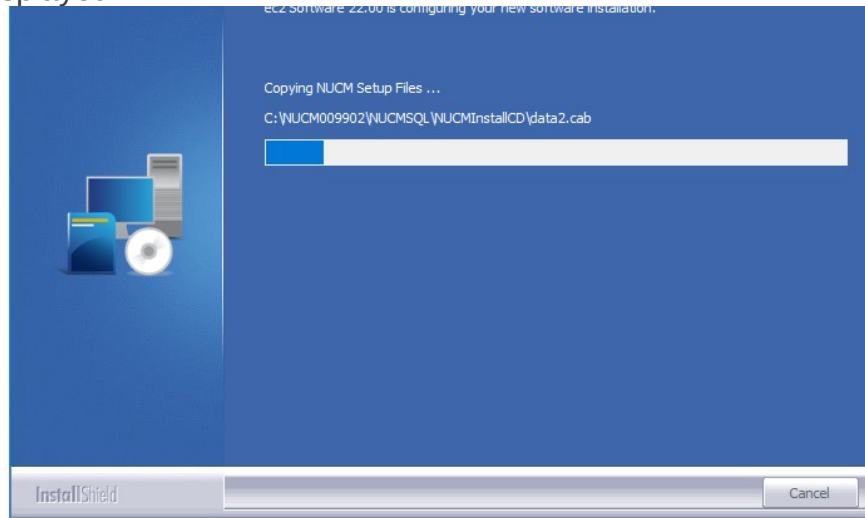

12. Next the program will install SQL Server if it is not already installed. **This part of the installation could take 15-30 minutes.**

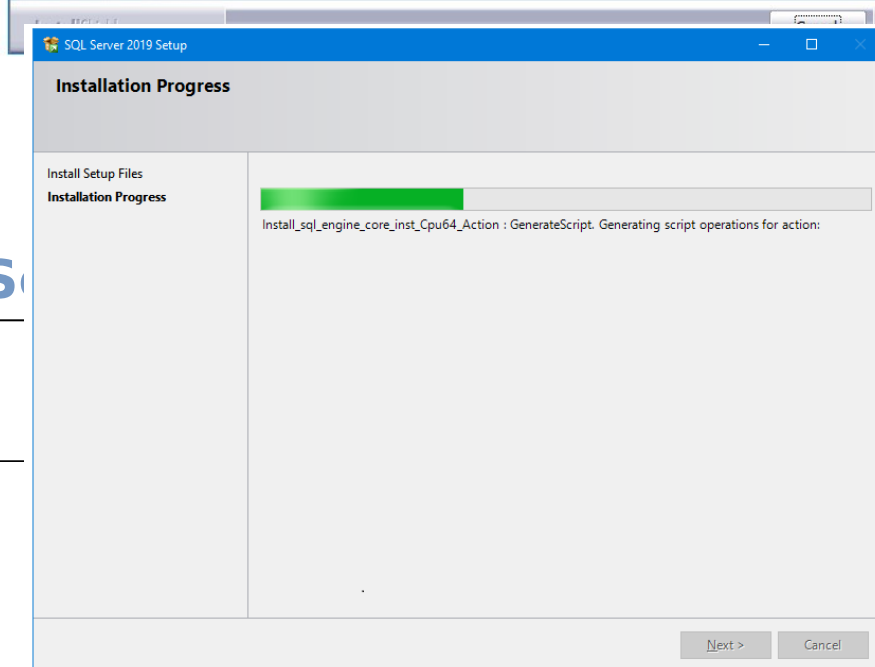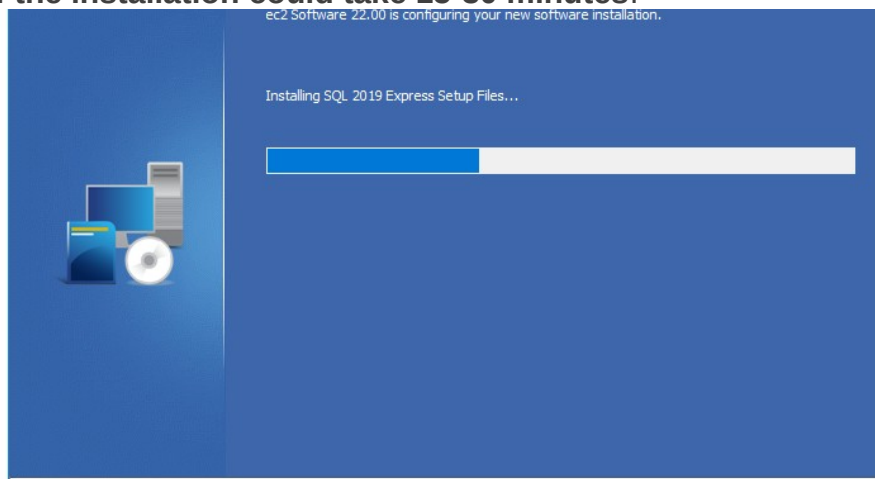


13. The program will then install any remaining applications not already installed. **This part of the installation could take up to 15 minutes.**

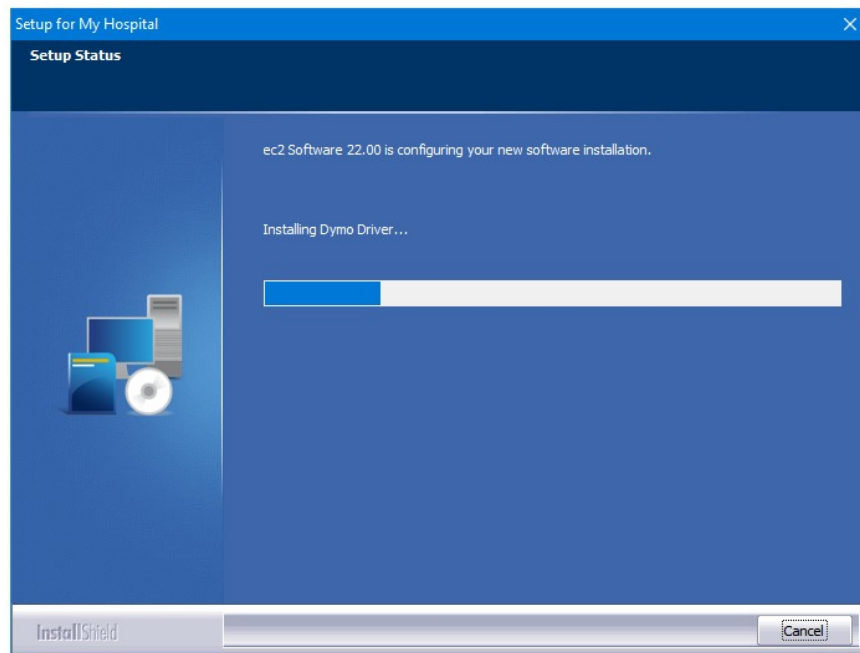


Server Installation (continued)

14. When the installation process has completed the below screen and message will be displayed. Click **OK** to continue.
-

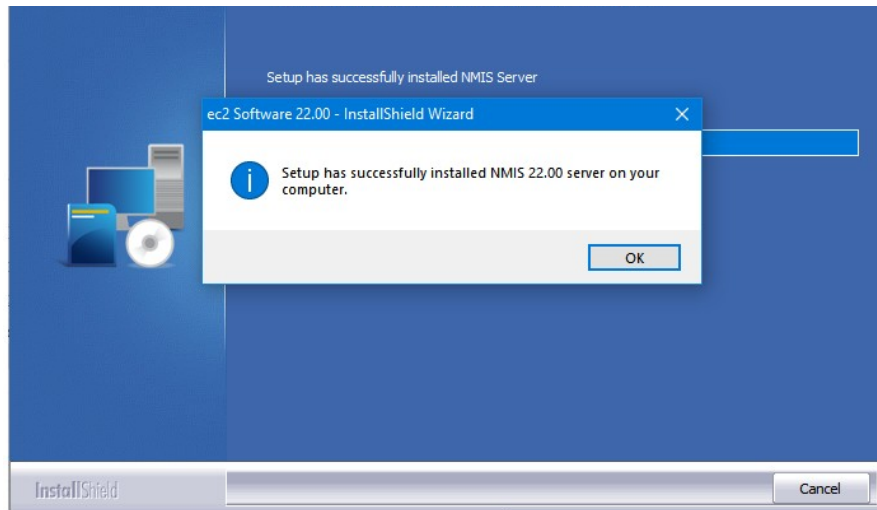


15. Once the database has been installed the below message will be displayed with the option to install this computer as a workstation. If someone will be using this computer to enter data click **Yes**. If this is a dedicated server and no one will be using it to enter data, click **No**.

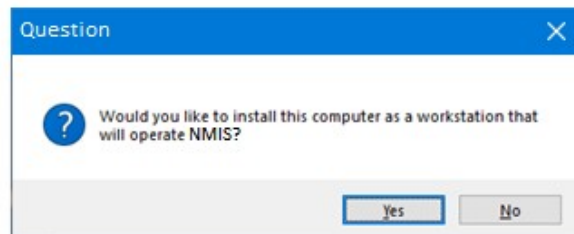

Server Installation (continued)

16. After restart the installation program will continue and display the below message when finished. Click **OK**.
-

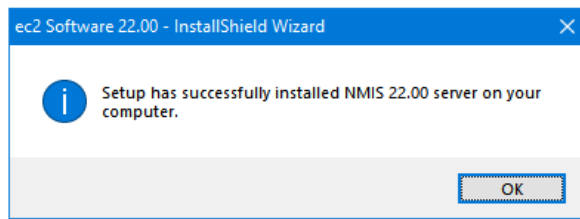


If you chose to make the server a workstation, you may now run NMIS 22.x using the desktop icon.


Workstation Installation

Note: You will not use the software disk to install the workstations.

1. Browse to the server and locate the `\\Server\NUCM#####\NUCMSQL\NUCMInstallCD` folder. Double-click on the `setup.exe` file.
2. On the **Welcome** screen, click **Next**.

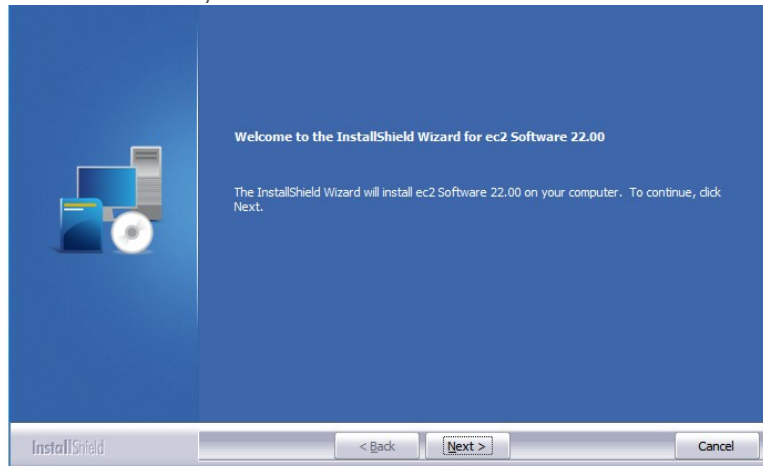


3. The installation program will examine your computer for all required components. If all required components are installed, you will move to step 5. If there are missing components, the below screen will be displayed listing them.

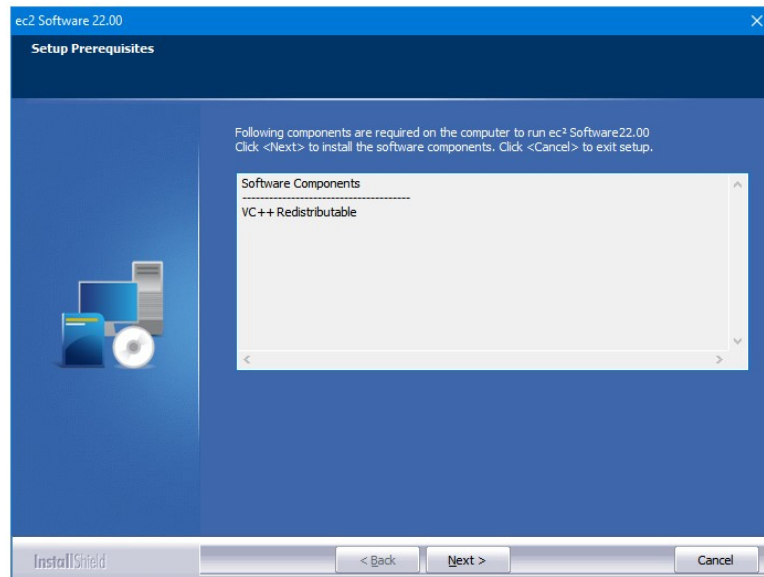


Workstation Installation (continued)

- The installation program will install the missing components. Once all components are installed, the **Welcome** screen will be displayed. Click **Next**.
- On the **License Agreement** screen select the **I accept the terms of the license agreement** radio button then click **Next**.

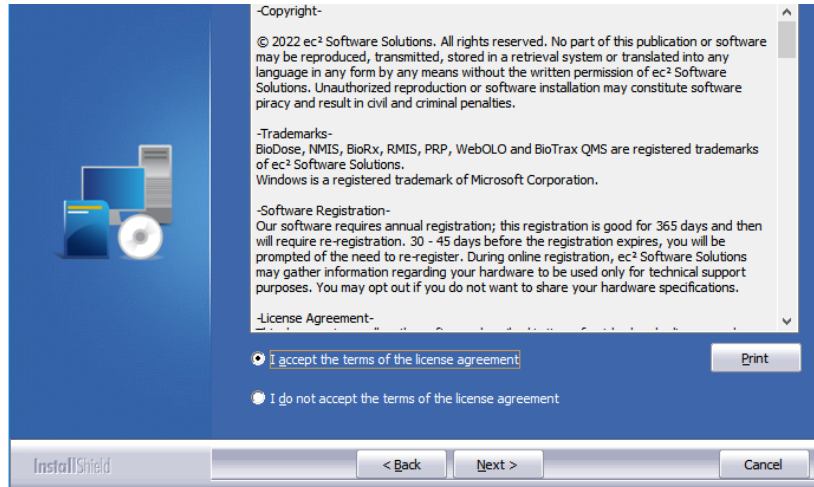


- Click **Yes** on the below message to start the installation.

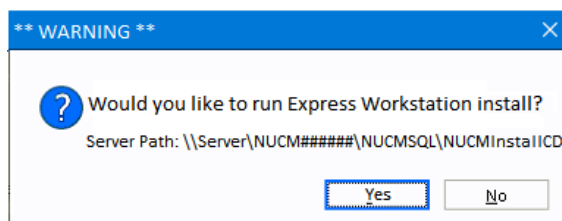


Workstation Installation (continued)

7. The program will copy the installation files while the below screen is displayed.

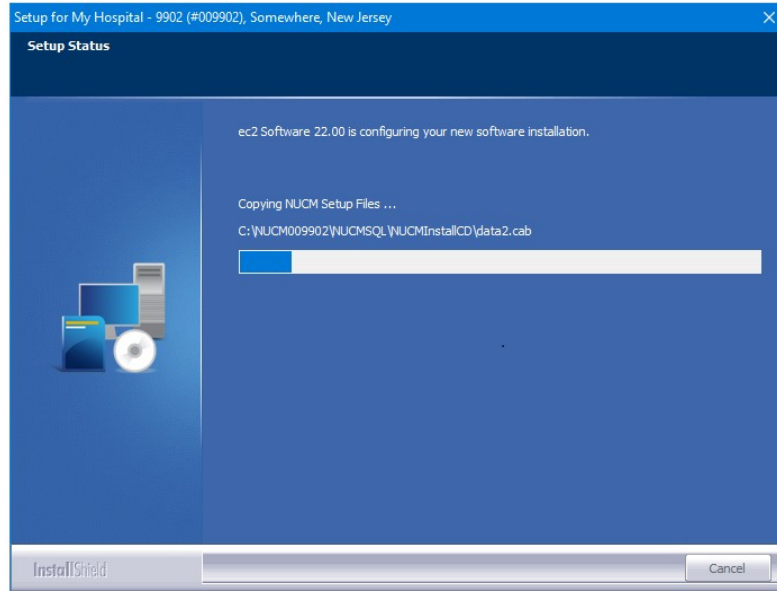

8. When the installation is completed the below screen and message will be displayed. Click **OK**.

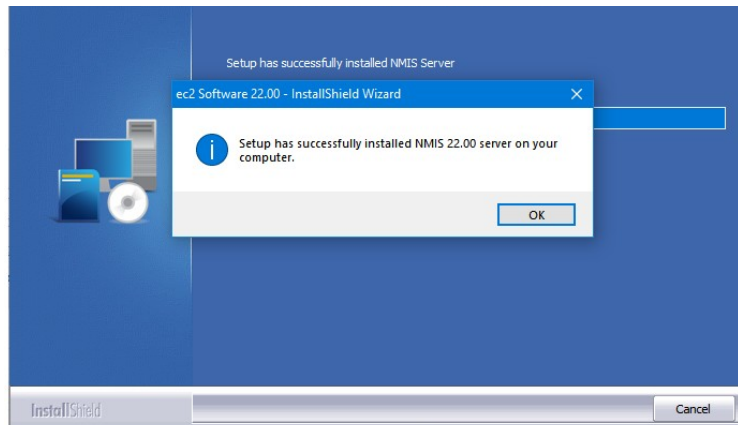

7. If a message is displayed requiring a restart, click **OK**.

Software Registration

What is Registration?

The software requires an annual registration for customer licensing validation. This is an internal tracking system that verifies that the software was installed in accordance with the license parameters. The first time you run the software you will see the below screen:

Initial NMIS Registration

You must register NMIS within 30 days.
If you don't register by then, the, NMIS will stop working.

You may Register by clicking <Register Online Now> button.

Customer Number: 0

First Name:

Last Name:

Phone:

Email:

[Auth ID](#)

Ways to Register

Register Online:

If you have Internet access, complete the above form and click **Register Online Now** to register your software.

Register Offline:

If you don't have Internet access call our [technical support](#) team to register your software. When you call we'll give you an Authorization ID.

When to Register

You have 30 days to register and each time you launch the software prior to registration the above screen will be displayed. Click **Register Later** to access the software prior to registration.

Note: If you register online there is nothing else to do. If you do not have Internet access, registration is independent upon renewing your annual software support and does not guarantee that you are eligible for software support.

Setup Instructions (continued)

Running the Start-up Wizard


If you have purchased on-site or web-based training, we will work with you to build the databases in the software. If you are anxious to get started, you can run the startup wizard which will guide you through building the databases. You can also use the wizard to add exams, radiopharmaceuticals or equipment at any time.

It is recommended that you select the **Startup Wizard** topics in order since some topics depend on the data from previous topics being complete. For example, dose calibrator constancy depends on both the dose calibrator and the sealed sources data being available.

1. Click **Help** on the menu bar.




2. Click

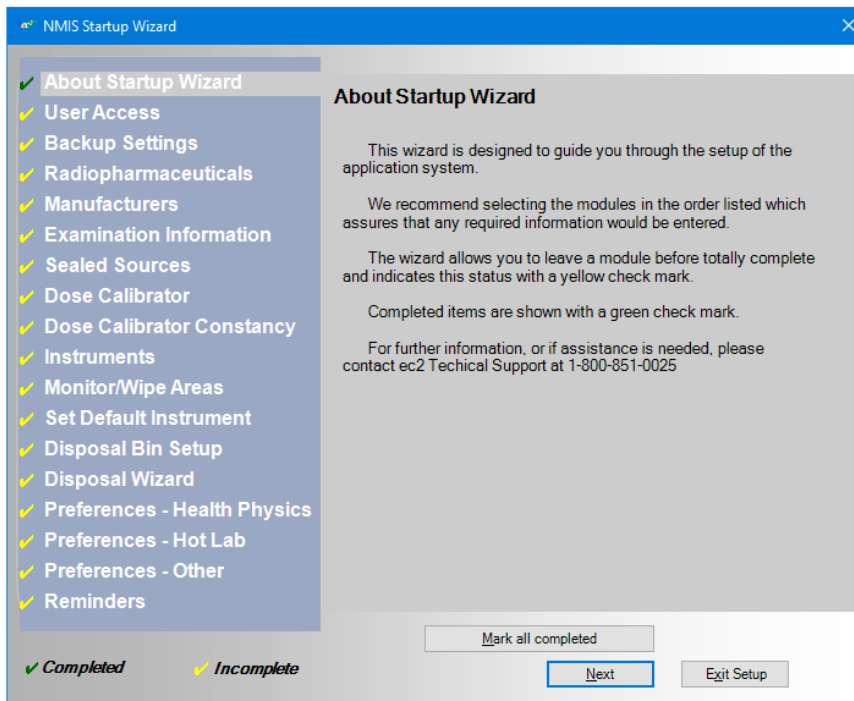

3. Click Next.

Setup Instructions (continued)

4. Select the first incomplete topic in the listing and click Setup.

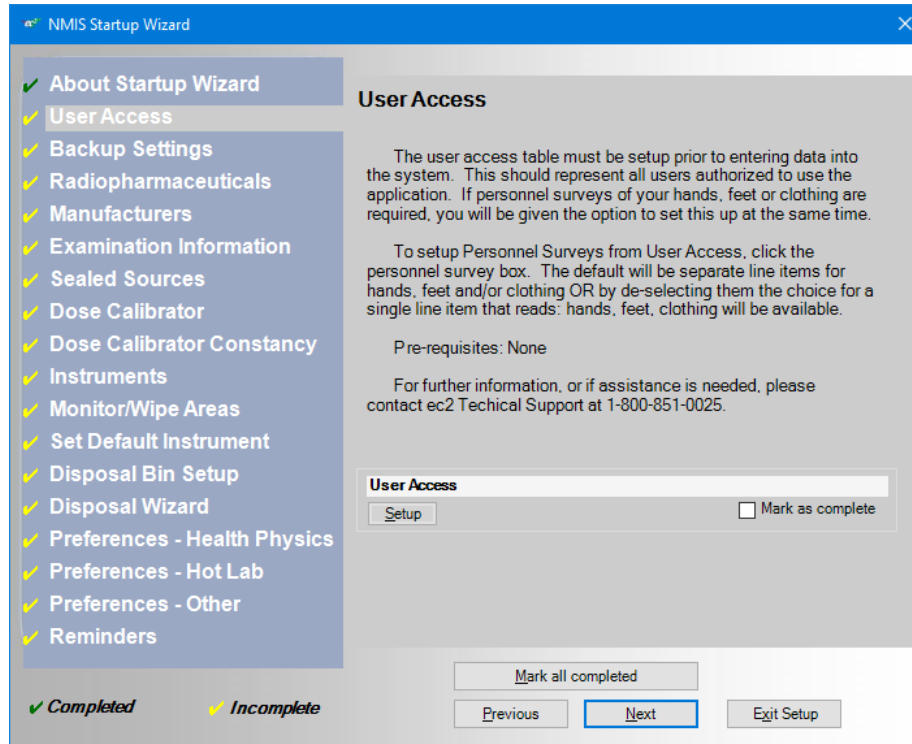



ec2software.com

400 Apgar Drive, Suite I, Somerset, NJ 08873

P: 800 851 0025 F 732 356 8746

E: info@ec2software.com



Nuclear Medicine Software

Version 22 Old to New BioDose Conversion

This section of the installation guide is intended for customers who are upgrading from an older version (4.08 or earlier) of BioDose software.

Pre-Installation Checklist

Before you Begin

Making sure that your hardware is adequate to run our software is extremely important. For [hardware requirements](#) information please refer to that section in this guide.


You should have received the BioDose version 22.x DVD along with this installation guide. Please that the facility name on the disk is correct. If it is not, please contact [technical support](#) before continuing.

Important Points

1. If you are running BioDose version 3.66 or earlier we will need to upgrade the databases first during the conversion in order to upgrade to version 22. The process will go much smoother if your existing BioDose is on the same computer you want to upgrade.
2. Shut down any programs that are running. Antivirus software can slow down the installation or prevent it from finishing.
3. Disable any screen savers that could disrupt the installation.
4. The software installation could take up to 60 minutes. Please give yourself plenty of time to complete the process.
5. You will be asked to restart your computer several times during the installation. Please restart whenever requested to do so.
6. You must be logged in as an administrator to install BioDose. It is important that you use the same administrator login after each restart until the program tells you the installation was successful.
7. For [server installation](#) and [workstation installation](#) instructions please refer to those sections in this guide.

Conversion Instructions

1. The conversion process to bring your data from BioDose version 3.x or 4.x will begin automatically after the installation finishes. The below screen will be displayed.

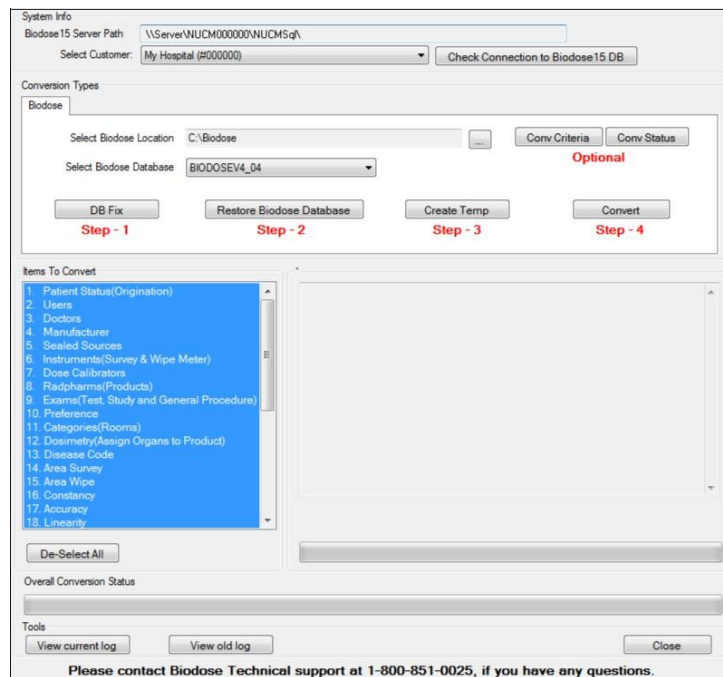

2. The conversion will run through the data and in most cases will be done in an hour. For the most part there will be nothing you have to do other than let it run.
3. When the program is converting the radiopharmaceuticals, if it finds a drug it doesn't understand it will ask you to either pick an equivalent drug from a list or possibly create a new one to match the way you had it set up in the old software.
4. Once the conversion completes, you can run BioDose from the desktop icon. The first workstation to run BioDose after the installation will complete the registration process for the entire facility. For [software registration](#) instructions, please refer to that section in this guide.

Contact Information

Need Technical Support?

We're always happy to help you! If you have any questions or concerns please contact *ec² Software Solutions* technical support. With your permission, we can log into your computer remotely, look at the screens with you and work through the issues together.

You can contact us Monday through Friday from 8:00 am - 8:00 pm EST.

By Phone: 800-851-0025 option 1

Fax: 732-356-8746

By Email: support@ec2software.com

